

An Optimized Low-Noise Low-Power Preamplifier for Cardiac ImplantsSanna Mairaj¹, Suhaib Ahmed^{1,*}, Vipan Kakkar¹

¹*Department of Electronics and Communication Engineering, Shri Mata Vaishno Devi University, Katra, J&K - 182 320, India.*

Abstract

Among various analog circuits, preamplifier has a prominent role in the analog front end (AFE) circuit of biomedical implantable microsystems for reliable acquiring of weak biophysiological signals. The AFE acts as an interface between the acquired analog biosignals and the digital part in these implants. As the industry of the biomedical implantable devices develops, lowering the power consumption as much as possible, without sacrificing the performance, is essential in improving the service time of the battery, which cannot be replaced frequently. Hence there is an increasing demand for a low noise, low power bio-acquisition system so as to avoid bulky connectivity and reduce patient mobility and discomfort. This paper thus presents an operational transconductance based preamplifier for application in cardiac implants. The performance of the proposed design has been evaluated based on various parameters such as gain, common mode rejection ratio (CMRR), noise spectral density, power consumption among others. Besides, the optimization by supply voltage scaling of the proposed design has also been done with focus on lowering the power consumption. The trade-offs between various parameters like gain, speed, power consumption are observed in the optimized design. The preamplifier, designed in 180nm CMOS technology, provides a high gain of 50dB at a supply voltage of 1.5V and a low power dissipation of 61.10 μ W. Based on the performance evaluation, it is observed that the proposed preamplifier is suitable for low power cardiac application.

Keywords: Cardiac Implants, Preamplifier, Low Power Electronics, Operational Transconductance Amplifier.

PACS: 84.30.Le, 84.30.-r, 85.40.-e, 87.55.tg, 87.85.Tu, 87.85.Ng

1. Introduction

The term implant represents a medical device that acts as a part of the whole biological system or can be used to provide support to a damaged biological structure [1,2]. Currently biomedical implants are used for various applications including cardiac pacemakers, defibrillators, cardiovascular stents etc. Monitoring of biomedical signals provides us information about the vital health of body and thus the data can be of prime importance to medical practitioners [3]. With the rapid development in microelectronics towards medical therapies and diagnostic aids, there is a need for lowering the power consumption in active implantable devices that are battery powered so that the device lifetime increases. One such example of active implantable device is the Cardiac Pacemaker in terms of its widespread application [4]. A Cardiac Pacemaker is a device that uses electrical pulses to recover the normal heartbeat of a diseased heart. The major building blocks of the pacemaker, shown in fig. 1, are analog front end (AFE) circuit,

*) For Correspondence, Tel: +(91) 9018807158, E-mail: sabatt@outlook.com

In Press, Accepted Manuscript – Note to users

microcontroller with ultra low power consumption, battery and an output circuit that stimulates the heart. The AFE comprises of a preamplifier, low-pass filter, level shifter, synchronizing circuit etc. The cardiac signal is given to a low noise preamplifier for amplification purposes and is then filtered. This filtered signal is then given to comparator that produces a pulse which depends upon the threshold voltage level. The output stage of a pacemaker is called a charge pump that uses a pulse generator to stimulate the activity of the heart. Thus a preamplifier is critical block that is used for the detection of the small level signals especially for the biomedical applications [3].

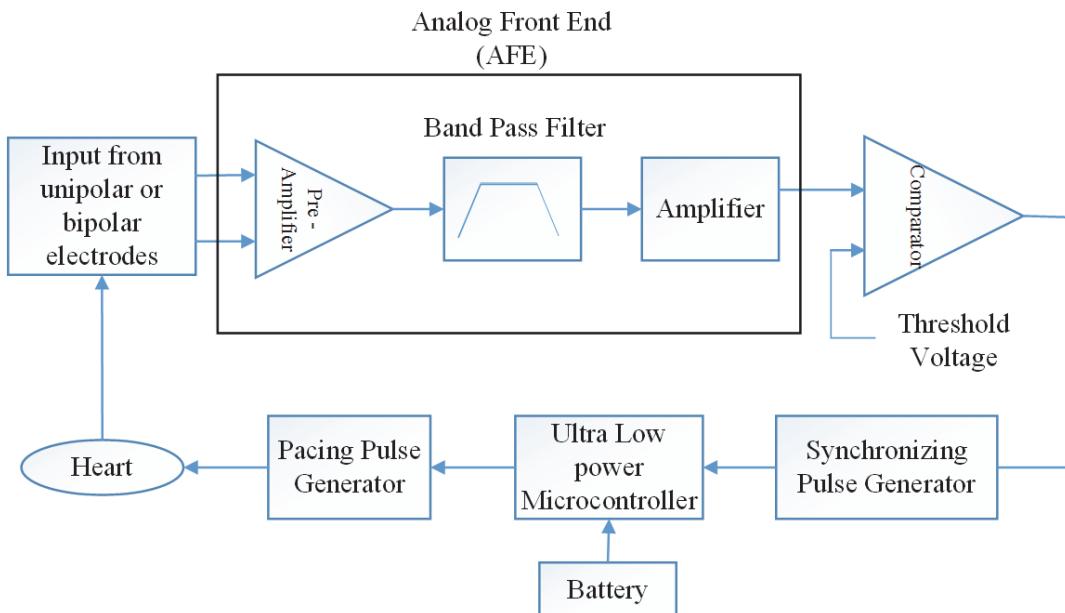


Fig. 1: General Block Diagram of an Implantable Cardiac Pacemaker System

The Biosignals like EEG, ECG, EMG, EOG are weak signals with input amplitude typically ranging from $0.5\mu V$ to $5mV$ [5,6] and are highly susceptible to noise and power line interference at 50Hz to 60Hz. Nowadays there is a demand for a low noise low power bio acquisition system so as to avoid bulky connectivity and reduce patients' mobility and discomfort [7]. A Preamplifier is one of the important component of the analog front end as it determines the SNR of the entire biomedical signal acquisition system and is required for reliable monitoring of the physiological signal [8]. These weak biosignals need to be amplified before being compatible for processing by the other components of the implant for measurement and testing purposes [9].

2. Design Specifications

Neural implantable devices, EEG and cochlear implants are the major application areas for preamplifier design in the survey [10-15] while less explored applications being cardiac pacemaker, EOG, PCG, retinal prostheses. The key design parameters of an amplifier are its Gain, stability, power consumption, CMRR, PSRR, Noise, THD, Dynamic range etc. Different applications demand different parameters that are critical to that particular application. Some applications like Neural Implantable devices require a low noise, low power analog front end while others like cochlear require a high PSRR, good

In Press, Accepted Manuscript – Note to users

SNR etc. Based on the literature study [16-18], the required design specifications for the preamplifier for Cardiac Implants are formulated and are summarized in table 1. A high gain of >50dB, high CMRR of around 70dB and high PSRR of a 60dB are required for this particular application.

Table 1: Design Specifications for Preamplifiers in Cardiac Implants

Parameters	Target Specifications
Gain	> 50dB
Slew Rate	>10V/ μ s
Load Capacitance	10pF
Min and Max Output voltages	\pm 2V
Unity Gain Bandwidth	7MEG
ICMR	-1.5V to 2.5V
CMRR	> 70dB
PSRR	> 60dB
Technology	180nm

3. Proposed Low Power Preamplifier

The folded cascode Operational Transconductance Amplifier (OTA) is chosen for the design of the preamplifier for cardiac applications. An OTA is actually an op-amp without output buffer and is capable of driving only capacitive loads. One of the important features of OTA is that its transconductance can be adjusted by a bias current. A folded cascode is actually a compromise between a two stage and telescopic cascode. The name “folded” comes from the fact that because of folding of P-channel cascode active loads of a differential pair and then converting the MOSFETs to N channel. A folded cascode overcomes the drawbacks of a telescopic structure i.e. limited output swings and difficulty in shorting input and output, thus provides wide swing. Wide Swing means an input Common mode range very close to the supply voltage [19]. The Output voltage swing is limited by supply voltages. In a folded cascode OTA a perfect balance of currents in the differential amplifier stage is not required because of the fact that excess dc current can flow in or out of the current mirror. The practical version of an OTA and its small signal Model are shown in fig. 2 and fig. 3 respectively. The bias currents I_3 , I_4 and I_5 of the topology should be designed such that the DC current in the cascode mirror never goes to zero e.g. if the input voltage V_{in} is made large enough such that M1 is turned on and M2 is turned off. Then all the current I_3 will flow through M1 that results in $I_1 = I_3$ and I_2 will be zero. If the currents I_4 and I_5 are not greater than current I_3 then I_6 will be zero. To avoid this problem the values of currents I_4 and I_5 are kept between values of currents I_3 and $2I_3$ [20]. The resistances R_A and R_B as seen looking into the source of M6 and M7 and are given as:

In Press, Accepted Manuscript – Note to users

$$R_A = \frac{rds_6 + R_2 + \frac{1}{gm_{10}}}{1 + gm_6 \cdot rds_6} \approx \frac{1}{gm_6} \quad (1)$$

$$R_B = \frac{rds_7 + R_9}{1 + gm_7 \cdot rds_7} \approx \frac{R_9}{gm_7 \cdot rds_7} \quad (2)$$

Here, $R_9 = gm_9 \cdot rds_9 \cdot rds_{11}$

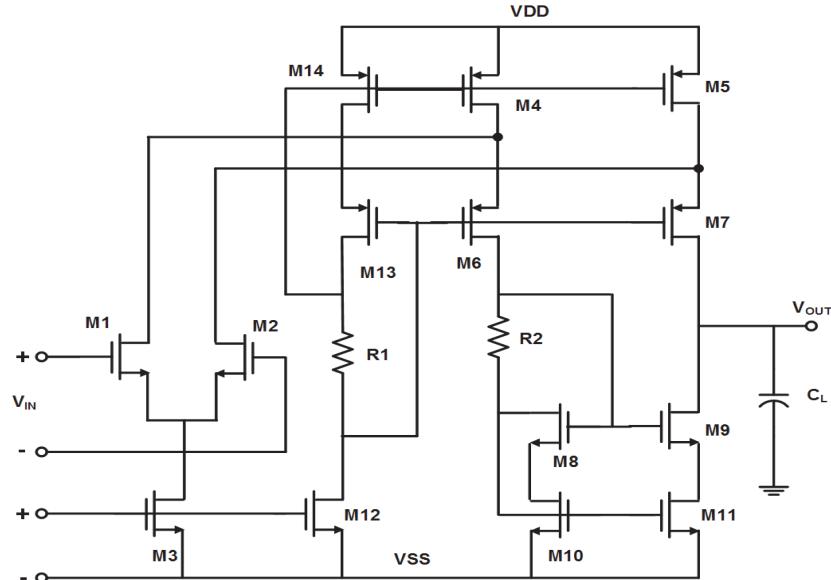


Figure 2: Folded Cascode OTA schematic

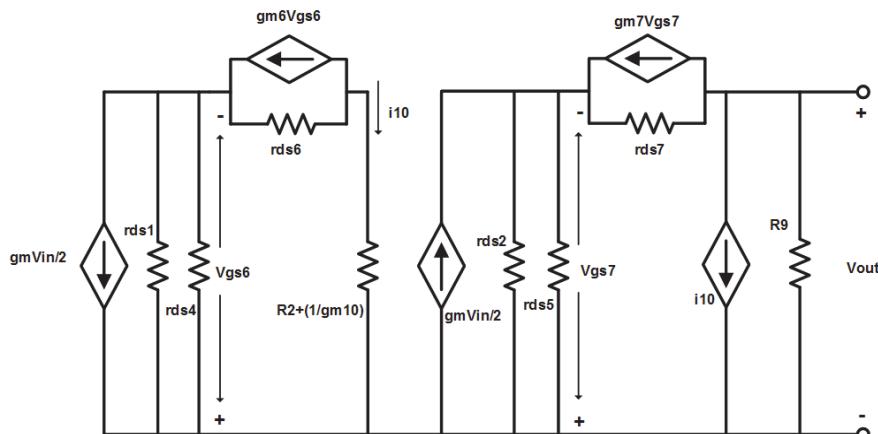


Figure 3: Small signal model of the OTA

Current i_{10} is given as:

$$i_{10} = \frac{-gm_1(rds_1 \parallel rds_4)V_{in}}{2(R_A + (rds_1 \parallel rds_4))} = \frac{-gm_1 \cdot V_{in}}{2} \quad (3)$$

Current i_7 can be written as:

In Press, Accepted Manuscript – Note to users

$$i_7 = \frac{gm_2 \cdot V_{in}}{2 \left(1 + \frac{R_9(gds_2 + gds_5)}{gm_7 \cdot rds_7} \right)} = \frac{gm_2 \cdot V_{in}}{2(1+K)} \quad (4)$$

Typically $K > 1$

$$K = \frac{R_9(gds_2 + gds_5)}{gm_7 \cdot rds_7} \quad (5)$$

The Output Voltage can be expressed as the sum of i_7 and i_{10} flowing through R_{11}

$$\frac{V_{out}}{V_{in}} = \left(\frac{gm_1}{2} + \frac{gm_2}{2(1+K)} \right) = \left(\frac{2+K}{2+2K} \right) gm_1 \cdot R_{11} \quad (6)$$

where R_{11} , the output resistance is given as $R_{11} \approx gm_9 \cdot rds_9 \cdot rds_{11} \parallel (gm_7 \cdot rds_7 (rds_2 \parallel rds_5))$

3.1 Analytical Modeling

The design of Proposed Folded Cascode OTA is done using level 49 BSIM3v3 MOSFET and TSMC 0.18μm T-Spice parameters are used which are summarized in table 2. The design consists of determining the specifications, selecting device sizes and biasing conditions, simulating and characterizing various performance parameters like open loop gain, CMRR, slew rate, output swing etc.

Table 2: Parameters from Tspice Model File (TSMC 180nm)

Parameter	Value
k_n'	$172.1 \mu\text{A}/V^2$
k_p'	$-36.4 \mu\text{A}/V^2$
Low Field Mobility μ_n	$398.72 \text{ (cm}^2)/\text{V*s}$
Low Field Mobility μ_p	$84.33 \text{ (cm}^2)/\text{V*s}$
V_{thn}	0.37965 V
T_{ox} for NMOS	4.1e-9 m
V_{thp}	-0.4215 V
T_{ox} for PMOS	4.1e-9 m

The main goal is to design a preamplifier based on above design specification and choosing proper W/L sizes for the amplifier design. The design steps to compute the transistor sizes are as follows :

1. Smallest device length is chosen such that the channel length modulation parameter λ is kept constant and also there is good matching for current mirrors. (Here $L=1\mu\text{m}$)
2. From the Slew rate expression the tail current I_3 is obtained

$$I_3 = SR \cdot C_L \quad (7)$$

Where SR is the slew rate, C_L is the load capacitance.

3. Bias currents in output cascode while avoiding zero currents in the cascode are given as

$$1.2I_3 \leq I_4 = I_5 \leq 1.5I_3 \quad (8)$$

In Press, Accepted Manuscript – Note to users

4. Design for S_5 and S_7 is obtained from the maximum output Voltage

Let $S_4=S_{14}=S_5=S_{13}$ and $S_6=S_7$

$$S_5 = \left(\frac{W}{L} \right)_5 = \frac{2I_5}{k_p \cdot (Vds_5)^2} \quad (9)$$

$$S_7 = \left(\frac{W}{L} \right)_7 = \frac{2I_7}{k_p \cdot (Vds_7)^2} \quad (10)$$

Here $Vds_5(\text{sat}) = Vds_7(\text{sat}) = \frac{V_{DD} - V_{out}(\text{max})}{2}$

5. Design for S_{11} and S_9 is obtained using minimum output voltage

Let $S_{10}=S_{11}$ and $S_8=S_9$

$$S_{11} = \left(\frac{W}{L} \right)_{11} = \frac{2I_{11}}{k_n \cdot (Vds_{11})^2} \quad (11)$$

$$S_9 = \left(\frac{W}{L} \right)_9 = \frac{2I_9}{k_n \cdot (Vds_9)^2} \quad (12)$$

Here $Vds_9(\text{sat}) = Vds_{11}(\text{sat}) = \frac{V_{out}(\text{min}) - |V_{ss}|}{2}$

6. Calculation of resistance values.

$$R_1 = \frac{Vds_{13}(\text{sat})}{I_{12}}, R_2 = \frac{Vds_8(\text{sat})}{I_6} \quad (13)$$

7. Design of S_1 and S_2 is obtained from the value of Unity gain bandwidth and load capacitance C_L .

$$S_1 = S_2 = \frac{GB^2 \cdot C_L^2}{k_n \cdot I_3} I_3 \quad (14)$$

Where $GB = \frac{gm_l}{C_L}$

8. S_3 design is Obtained from the minimum Input common mode voltage

$$S_3 = \left(\frac{W}{L} \right)_3 = \frac{2I_3}{k_n \left[V_{in}(\text{min}) - V_{ss} - V_{t1} - \sqrt{\frac{I_3}{k_n \cdot S_1}} \right]} \quad (15)$$

9. S_4 and S_5 design is Obtained from the maximum Input common mode voltage.

$$S_4 = S_5 = \frac{2I_4}{k_p [V_D - V_{in}(\text{max}) + V_{t1}]^2} \quad (16)$$

Also S_4 and S_5 values should be large enough to satisfy the maximum Input common mode voltage.

In Press, Accepted Manuscript – Note to users

10. The differential Voltage gain is given as

$$A_v = \left(\frac{2+K}{2+2K} \right) g_m \cdot R_{11} \cdot I_3 \quad (17)$$

11. Power dissipation given as

$$P_{diss} = (V_{DD} - V_{SS}) \cdot (I_3 + I_{12} + I_{10} + I_{11}) \cdot I_3 \quad (18)$$

12. Positive CMR given as:

$$V_{in}(\max) = V_{DD} - \left[\frac{I_5}{\beta_3} \right] \cdot |V_{TO3}|_{\max} + V_{T1}(\min) \quad (19)$$

13. Negative CMR

$$V_{in}(\min) = V_{SS} + V_{ds5}(\text{sat}) + \left[\frac{I_5}{\beta_1} \right]^{0.5} + V_{T1}(\max) \quad (20)$$

14. The second stage resistance is

$$R_1 = R_9 \parallel g_m \cdot \frac{1}{gds_7} \cdot \left(\frac{1}{gds_2} \parallel \frac{1}{gds_5} \right) \cdot I_3 \quad (21)$$

Where $R_9 \approx g_m \cdot rds_9 \cdot rds_{11} \cdot I_3$

15. The parameters can be evaluated from the following equations

$$gm = I_3 \cdot \sqrt{2 \cdot k_{n,p} \cdot S_{n,p} \cdot I_D} \quad (22)$$

$$gds = \lambda I_D \quad (23)$$

$$rds = \frac{1}{gds} = \frac{1}{\lambda I_D} \quad (24)$$

$$V_{ds}(\text{sat}) = I_3 \cdot \sqrt{\frac{2I_{DS}}{\beta}} \quad (25)$$

From the above mathematical equations the bias currents and the transistor sizes ($\frac{W}{L}$) for the amplifier are calculated and summarized in the Table 3, 4 respectively.

Table 3: Parameter Values

I_3	100 μ A
$I_4=I_5$	125 μ A
C_L	10pF
$R_1=R_2$	2K Ω

Table 4: Calculated $\frac{W}{L}$ of transistors (Assuming L=1 μ m)

W/L ratios of transistors	Transistor Widths (μ m)
---------------------------	------------------------------

$S_5 = S_4 = S_{14} = S_{13} = 109.80$	$W_5 = W_4 = W_{14} = W_{13} = 109.80$
$S_6 = S_7 = 65.93$	$W_6 = W_7 = 65.93$
$S_8 = S_9 = S_{10} = S_{11} = 47.44$	$W_8 = W_9 = W_{10} = W_{11} = 47.44$
$S_1 = S_2 = 11.24$	$W_1 = W_2 = 11.24$
$S_3 = 8.421$	$W_3 = 8.421$
$S_{12} = 10.5$	$W_{12} = 10.5$

3.2 Circuit Schematic

The proposed preamplifier schematic is shown in fig. 4. The topology uses cascode current mirrors as active biasing elements. Current mirrors are more economical than passive resistors in terms of die area required to provide bias current of a certain value.

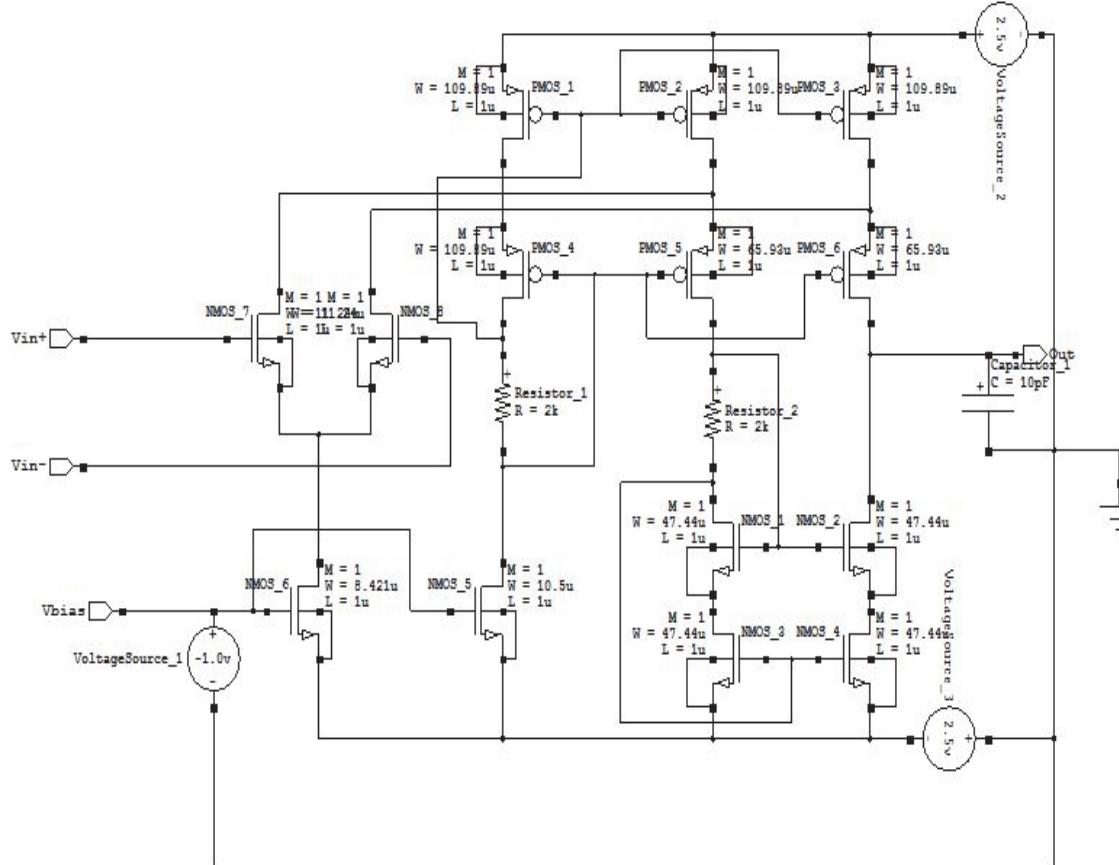


Fig. 4: Schematic of the proposed folded cascode OTA based preamplifier

A cascode current mirror provides a wider swing compared to a Wilson current mirror. Therefore because of this current mirror, folded cascode op-amp has a wider output swing. The 3 main stages of the OTA include differential input stage, folded cascode load stage and the output stage. The Cascode topology increases the gain of the input differential stage. Folded cascode is used to improve the ICMR and also to reduce the required supply voltage whereas, the Current mirror sink used in this folded cascode topology has following advantages:

- High Output resistance
- Low Power dissipation
- Self-biasing
- High swing
- Small saturation Voltage

4. Results and Discussions

Low Voltage and low power are important attributes for cardiac implants to achieve a longer battery life time. The proposed preamplifier is first designed at supply of 2.5 V and then optimized by scaling down to 1.5V to achieve lower average power consumption. To find the AC response of the OTA 100mV input is given to the differential amplifier along with DC voltages and the ac analysis is done from 1Hz to 10MHz. Fig. 5 shows the frequency response of the proposed designs.

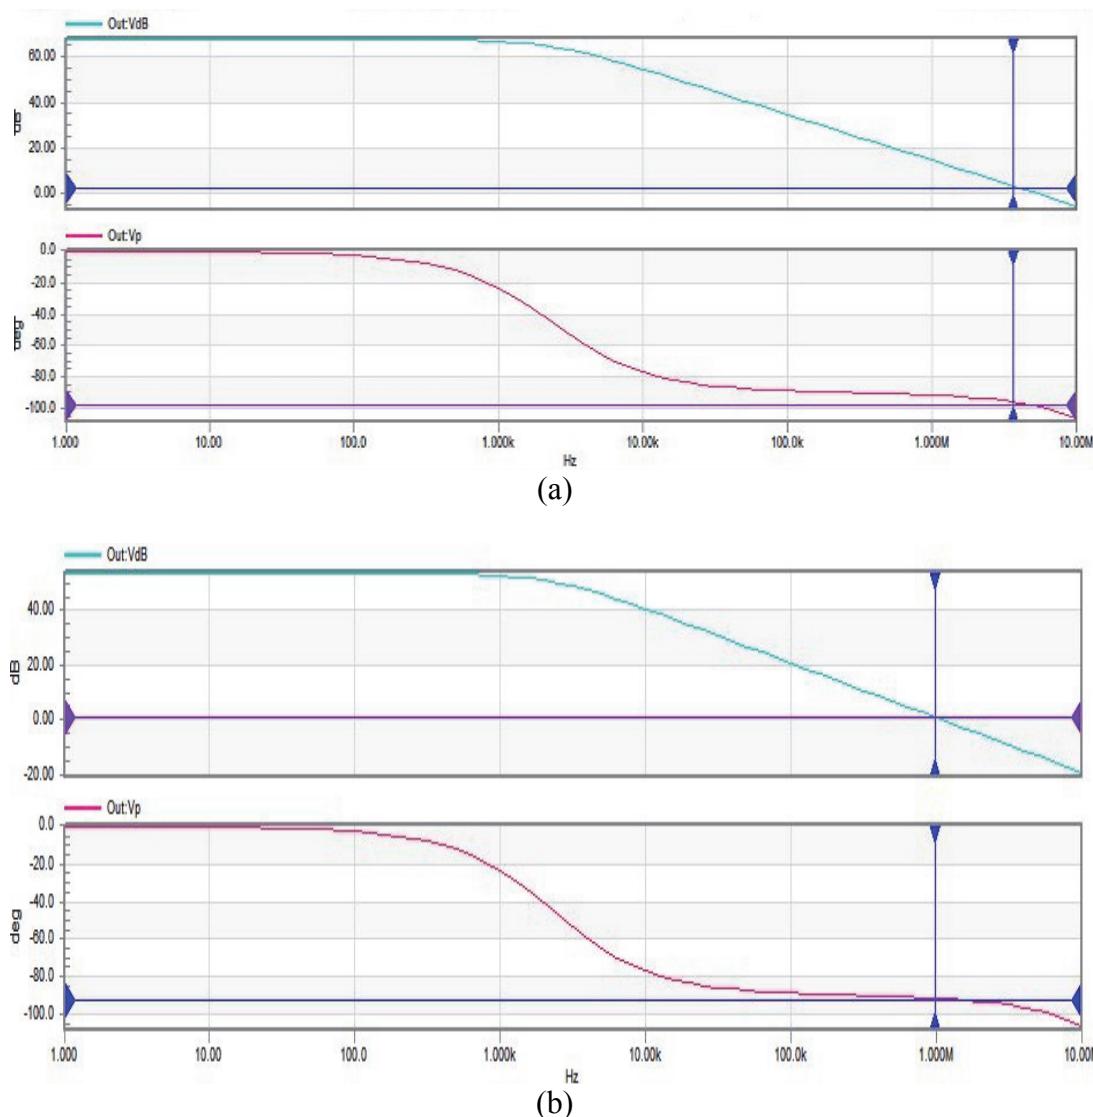


Fig. 5: Frequency response of the proposed preamplifier at (a) 2.5V and (b) 1.5V supply voltage

In Press, Accepted Manuscript – Note to users

To find Common Mode gain both the inputs V_{in+} and V_{in-} are shorted and AC voltage and DC are applied. The simulated results in Fig. 6 shows the common mode gain.


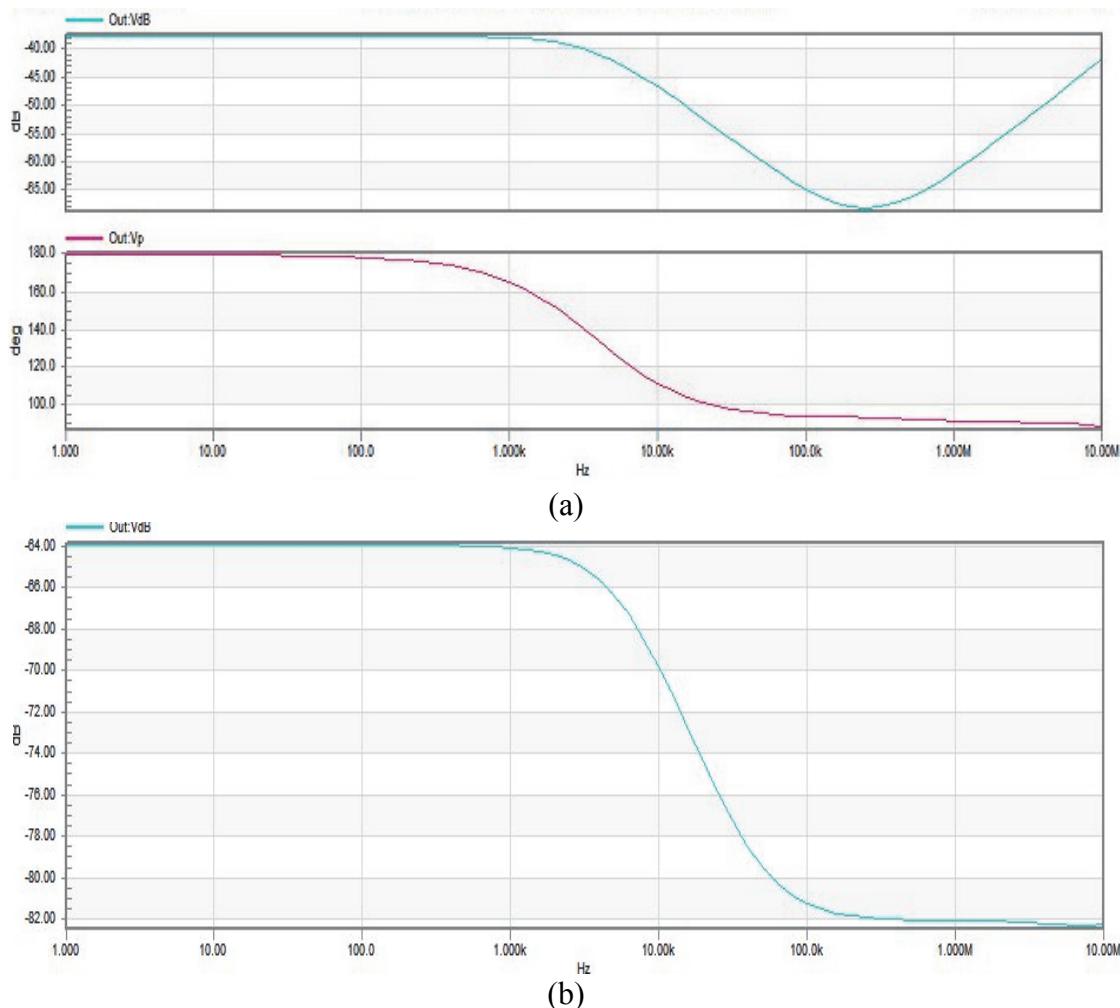


Fig. 6: Common mode gain at (a) 2.5V and (b) 1.5V supply voltage

A square wave is given to inputs of the differential stage and the transient analysis gives the simulation results. The Slew rate actually represents the current available to drive the load capacitance. The slew rate for the proposed designs can be evaluated from Fig. 7.

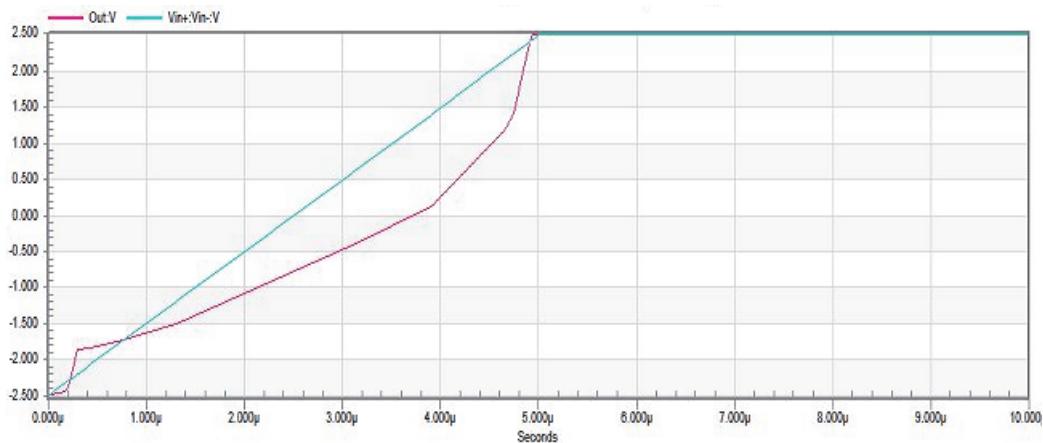

In Press, Accepted Manuscript – Note to users

Fig. 7: Slew rate at 2.5V

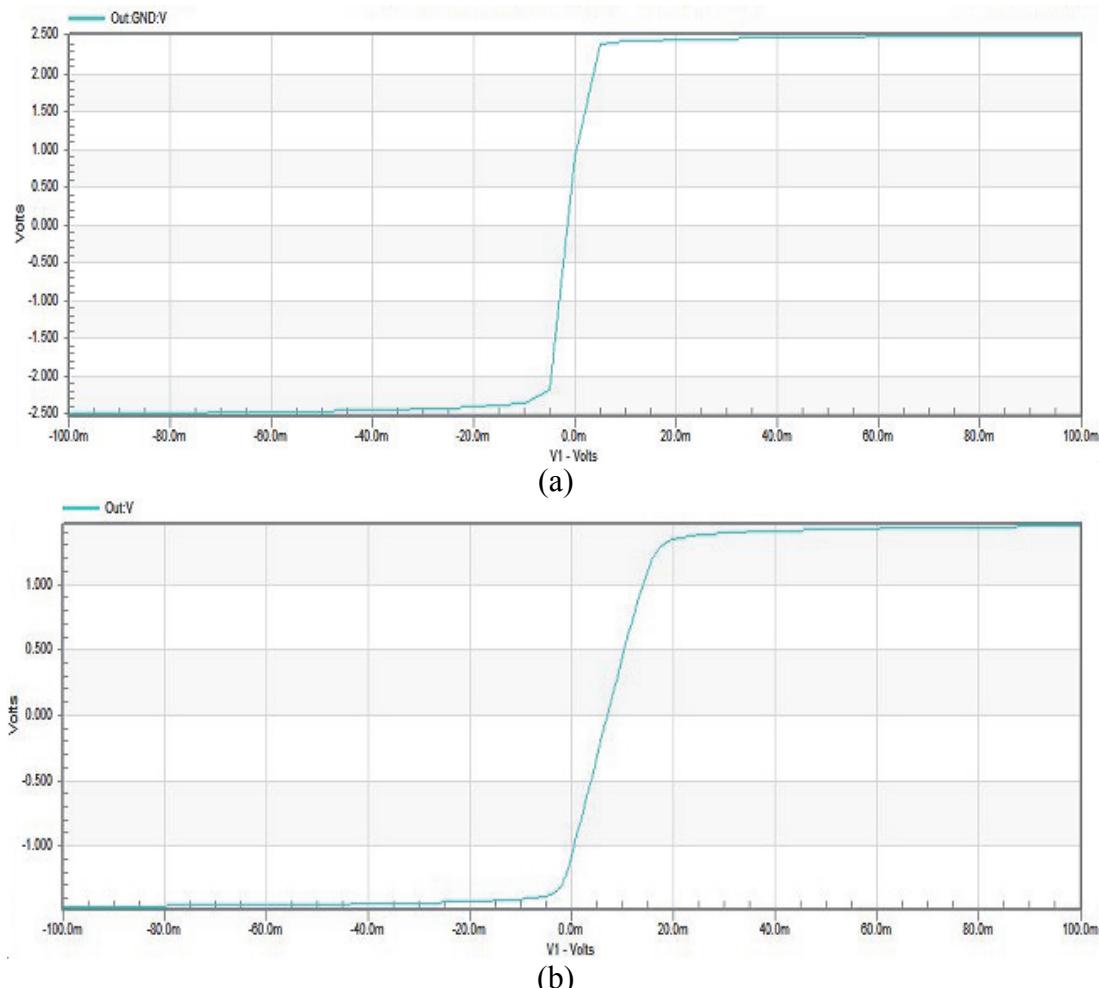


Fig. 8: Output swing at (a) 2.5V and (b) 1.5V supply voltage

Output swing represents the values of maximum positive and negative voltages above which transistor will remain out of saturation and thus specifies the range over which output voltage can vary without excessive distortion. The graphs in Fig. 8 shows the voltage swing from -2.5V to +2.5V. The OTA provides a wide swing meaning the input CMR is close to the supply voltages. The output swing is limited by supply voltages as is evident from Fig. 8..

In Press, Accepted Manuscript – Note to users

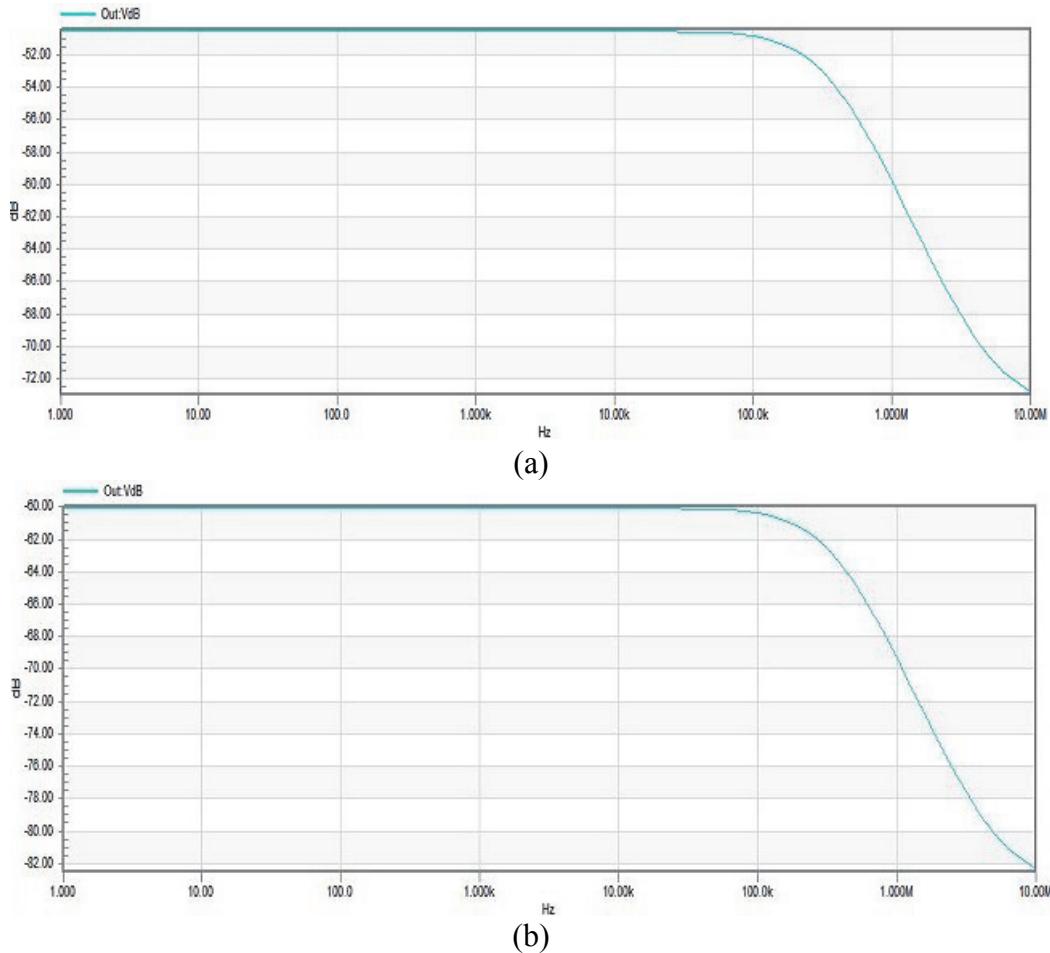


Fig. 9: PSRR at (a) 2.5V and (b) 1.5V supply voltage

If there is a change X in the supply voltage that produces an output voltage change of Y volts, then PSRR is expressed as a ratio of X/Y. This quantity is expressed in dB. PSRR can be positive or negative quantity. For finding the PSRR, DC bias is applied to inputs of the differential stage and an AC Voltage is applied to positive V_{DD} terminal to find PSRR +. For the proposed designs, the PSRR can be calculated from the graph shown in Fig. 9.

This paper first presents the design of a preamplifier for cardiac implants designed at supply voltage of 2.5V and a high gain of around 60dB is obtained but the power consumption is slightly high. Therefore further optimization is done and results at supply voltage of 1.5V are obtained. The average power consumption reduces to $61.10\mu\text{W}$ but at the expense of reduced gain of 50dB. Also there is an improvement in the noise spectral density at 1.5V. The performance parameters of the proposed and optimized deisngs are summarized in table 5.

Table 5: Comparsion of Proposed and Optimized Preamplifier Designs

Specification	Proposed Design	Optimized Design
Supply Voltage	2.5 V	1.5V
Open Loop Gain	62dB	50dB

In Press, Accepted Manuscript – Note to users

Phase Margin	-95.83°	-92.02°
CMRR	102dB	114dB
PSRR+	-50dB	-60dB
Power Consumption	0.131mW	61.10μW
Output Swing	-2.5V to 2.5V	-1.4V to 1.4V
Noise Spectral Density	250μV/ \sqrt{Hz} at 100mV input	3.5μV/ \sqrt{Hz} at 100mV input

The state of art comparison of the proposed low power preamplifier with some other related work is given in Table 6. A gain of 50dB, a low power consumption of 61.10 μW, a high CMRR of 94dB is achieved which is suitable for the cardiac applications. Also an improvement in the noise spectral density is quite evident from the table.

Table 6: Performance Comparison of Proposed Preamplifier

Parameter	[21]	[22]	[23]	[24]	This Work
Technology (μm)	0.6	0.35	0.18	0.18	0.18
Gain (dB)	39.4	20.4	40	63.06	50
Power Consumption (W)	2.4μ	23.1μ	-	0.0154m	61.10μ
CMRR (dB)	66	-	82	-	114
PSRR (dB)	80	-	-	-	60
Supply Voltage (V)	2.8	3.3	1.8	1.8	1.5

5. Conclusion

The parameters like size, weight, battery are of prime importance in cardiac implants. As the industry of the medical implantable devices develops, lowering the power consumption as much as possible is essential in improving the service time of the battery, which cannot be replaced frequently. Hence low voltage operation becomes critical for achieving low power consumption .This paper presents the design and optimization of an OTA based preamplifier for cardiac application. The preamplifier provides a gain of 50dB at a supply voltage of 1.5V and a low power dissipation of 61.10μW thereby making it suitable for this particular application and the trade-offs between various parameters like gain, power consumption are also evident in the optimized design. In future, further optimization to ultra-low power level can be done. Also different applications like retinal prostheses, EOG, PCG, etc. can be considered since much of the work is done on neural implantable devices.

In Press, Accepted Manuscript – Note to users

References

- [1] W. Khan, E. Muntimadugu, M. Jaffe, A.J. Domb, Implantable Medical Devices, Focal Controlled Drug Delivery, Springer (2014) 33-59.
- [2] R.J. Baker, Current Mirrors, CMOS Circuit Design, Layout, and Simulation, Wiley Student Edition (2005) 613-657.
- [3] F. Moulahcene, N.E. Bouguechal, Y. Belhadji, A Low Power Low Noise Chopper Stabilized Two Stage Operational Amplifier for Portable Bio-potential Acquisition Systems using 90nm Technology, International Journal of Hybrid Information Technology, **7** (2014) 25-42.
- [4] F. Silveira, D. Flandre, Implantable Cardiac Pacemaker, Low Power Analog CMOS for Cardiac Pacemakers, Design and optimization in Bulk and SOI Technologies, Kluwer Academic Publishers (2004) 1-24.
- [5] S. Ahmed, V. Kakkar, Modeling and Simulation of an Eight-bit Auto-Configurable Successive Approximation Register Analog-to-Digital Converter for Cardiac and Neural Implants, Simulation: Transactions of the Society for Modeling and Simulation International (2017) p. 0037549717716537.
- [6] S. Ahmed, S. Bashir, B. Bilal, V. Kakkar, Feasibility of Successive Approximation Register ADC in Ultra Low Power Biomedical Applications, International Journal of Engineering and Technology, **9** (2017) 338-347.
- [7] R. Chebli, M. Sawan, Low Noise and High CMRR Front-End Amplifier Dedicated to Portable EEG Acquisition System, Proc. of 36th Annual International Conference of the IEEE EMBS, (2013) 3-7.
- [8] S. Kumaravel, K.N.B. Tirumala, B. Venkataramani, R. Raja, A Power Efficient Low Noise Preamplifier for Biomedical Applications, Journal of Low Power Electronics, **9** (2013) 501-509.
- [9] J.H. Nagel, Biopotential Amplifiers, Biomedical Engineering Han-dbook, 2nd Ed., CRC press LLC (2000) 2-15.
- [10] J. Holleman, B. Otis, A Sub-Microwatt Low-Noise Amplifier for Neural Recording, Proc. of 29th Annual International Conference of IEEE EMBS, (2007) 23-26.
- [11] R. Reiger, J. Taylor, N. Donaldson, Low Noise Preamplifier Design for Nerve Cuff Electrode recording systems, Proc. of IEEE International Symposium on Circuits and Systems, (2002) 193-V-196-V.
- [12] M.-Z. Li, K.-T. Tang, A Low-Noise Low-Power Amplifier for Implantable Devices for Neural Signal Acquisition, Proc. of 31st Annual International Conference of the IEEE EMBS, (2009) 2-6.
- [13] R.R. Harrison, C. Charles, A Low-Power Low Noise CMOS Amplifier for Neural Recording Applications, IEEE Journal of Solid-State Circuits, **38** (2003) 958-965.
- [14] W.A. Serdijn, A.C. van der Woerd, J. Davidse, A.H.M. van Roermund, A Low-Voltage Low-Power Fully-Integratable Front-End for Hearing instruments, IEEE Transactions on Circuits and Systems - Fundamental Theory and Applications, **42** (1995) 166-169.
- [15] V. Kakkar, S. Ahmed, S. Koul, An Enhanced Pre-Amplifier for Cochlear Implants, Acta Technica Napocensis : Electroncia and Telecommunicatii, **56** (2015) 13-17.
- [16] A. Gerosa, A. Maniero, A. Neviani, A Fully Integrated Two-Channel A/D Interface for the Acquisition of Cardiac Signals in Implantable Pacemakers, IEEE Journal of Solid-State Circuits, **39** (2004) 1083-1093.
- [17] L. Fay, V. Misra, R. Sarpeshkar, A Micropower Electrocardiogram Amplifier, IEEE Transactions on Biomedical Circuits and Systems, **2** (2009) 312-320.

In Press, Accepted Manuscript – Note to users

- [18] K. Lasanen, J. Kostamovaara, A 1-V Analog CMOS Front End for Detecting QRS Complexes in a Cardiac Signal, IEEE Transactions on Circuits and Systems - Regular Papers, **52** (2005) 2584-2594.
- [19] B. Razavi, Operational Amplifiers, Design of Analog CMOS Integrated Circuits, Tata McGraw-Hill Publishing Company Limited (2002) 47-99.
- [20] M.H. Zarifi, J. Frounchi, S. Farshchi, J.W. Judy, A Low-power, Low Noise Neural Signal Amplifier Circuit in 90nm CMOS, Proc. of 30th Annual International IEEE EMBS Conference, (2008) 20-24.
- [21] C. Qian, J. Parramon, E. Sanchez-Sinencio, A Micropower Low-Noise Neural Recording Front-End Circuit for Epileptic Seizure Detection, IEEE Journal of Solid-State Circuits, **46** (2011) 1392-1405.
- [22] Z. Xu, P. Weihua, H. Beiju, Low Power CMOS Preamplifier for Neural Recording Applications, Journal of Semiconductors, **31** (2010) 045002.
- [23] J. Xu, R.F. Yazicioglu, P. Harpe, K.A.A. Makinwa, C.V. Hoof, A 160 μ W 8-Channel Active Electrode System for EEG Monitoring, IEEE Transactions on Biomedical Circuits and Systems, **5** (2011) 555-567.
- [24] D. Basak, P.V. Nishanth, R. P. Paily, A Low Noise Preamplifier and Switched Capacitor Filter for Heart-rate Detection, Proc. of International Conference on Advanced Electronic Systems, (2013).